

T80 Universal Transmitter

S80 Intelligent Sensors






T80 Universal Transmitter

❖ One Transmitter for Multiple Measurements

- pH
- ORP
- Dissolved Oxygen
- All Specific Ions
- Conductivity
- Resistivity
- Turbidity





T80 Universal Transmitter

- ❖ Easy to Use
- ❖ Membrane Switch Navigation
- ❖ Simple Menu Structure
- ❖ Soft Key Menu Choices
- ❖ Easy to read 2 3/4" x 1 1/2" LCD Display





T80 Universal Transmitter

- ❖ Inputs:
 - Any S80 Intelligent Sensor
 - Single or Dual Channel
- ❖ Outputs:
 - (1) or (2) 4-20 mA
 - MODBUS RTU on Line powered instruments
 - Optional HART® 7
 - Optional 3 Alarm Relays
- ❖ Power requirements:
 - Loop Powered
 - 24 VDC @ 250 mW minimum
 - 110/220 VAC



HART 
COMMUNICATION PROTOCOL





S80 Intelligent Sensors

- ❖ New but Familiar
- ❖ Digital Communication with Transmitter
 - Sensor Type
 - Serial Number
 - Process Variable
 - Temperature
 - Calibration Data
- ❖ Waterproof, IP68 rated Industrial Detachable Cable Connection





S80 Intelligent Sensors

❖ 6 Point Advantage

1. Intelligent Sensor
2. Common Configuration for all Measurements
3. Application Specific Cartridges
4. Economic and Easily Replaceable Cartridges
5. Submersible and Retractable designs
6. Application Specific Materials of Construction






T80 Home Display

❖ Three Home Screens


- Data Screen
 - Process Variable
 - % 4-20 mA range
 - Temperature
- mV Screen
 - Raw mV signal from the sensor
 - % 4-20 mA range
 - Temperature
- Graphical Screen
 - 3 choices, Line, Bar, Gauge
 - Process Variable
 - % 4-20 mA range

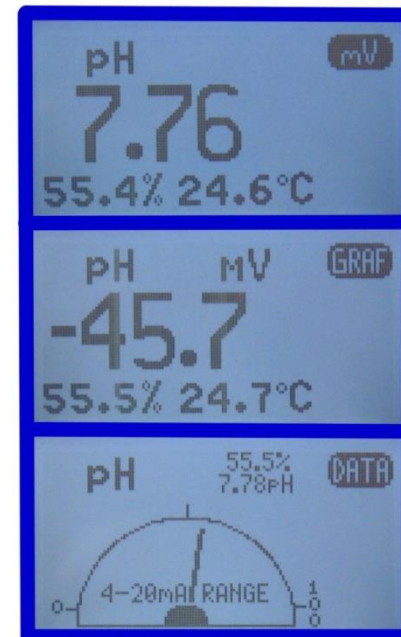



T80 Main Menu

- ❖ Press any Key Twice, except the Screen Key, within 1 second to enter the Main Menu
 - CAL = Calibration
 - CONFIG=Configuration
 - INFO = Information
 - SIM = Simulation
 - HOLD = Output Hold Function
 - Toggles ON/OFF
 - Freezes the 4-20 mA and alarm relays

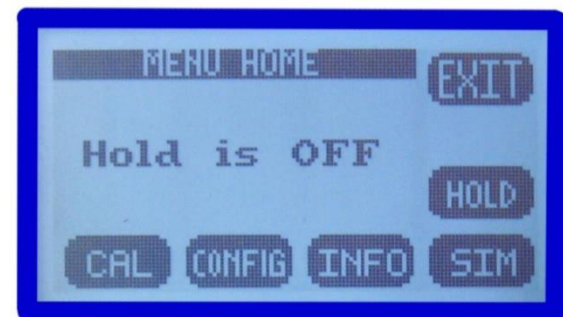



T80 Calibration


- ❖ New Sensor?
 - YES- Erases all 3 Calibration registers
 - NO- Saves to top register
- ❖ Auto Calibration
 - Two point Cal
 - Automatically recognizes the Calibration Solution
- ❖ Standardize
 - Single point adjustment
- ❖ Manual
 - User entry of the Offset and Slope for sensor
- ❖ Temperature
 - Temperature Adjustment






T80 Auto Calibration


- ❖ The Easy to use T80 prompts the user through the calibration.
- ❖ Press AUTO and Cal 1 and the T80 waits for a stable reading and then
- ❖ Suggests the value of the Calibration Standard
- ❖ Accept the value (YES) or enter a different value (NO)
- ❖ Continue to the next solution (YES) or end the calibration (NO).

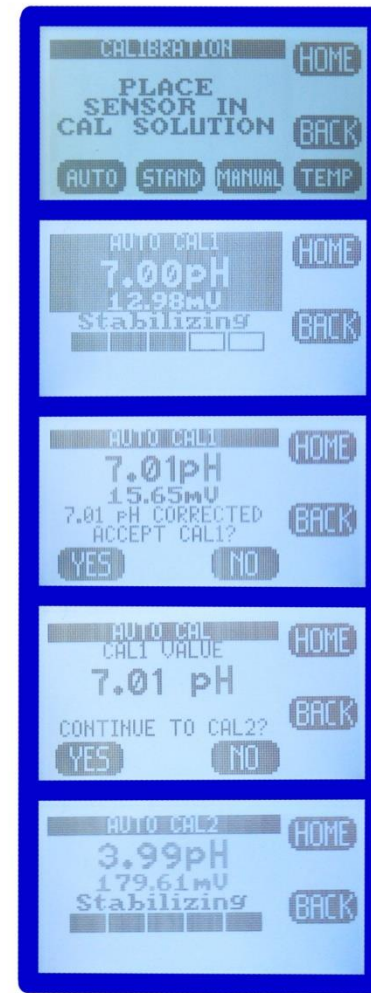




T80 Auto Calibration

- ❖ The 2nd standard solution is suggested when the sensor stabilizes
- ❖ Accept the value or enter a different one
- ❖ The Calibration Offset and Slope values are displayed
- ❖ Press OK to exit the Calibration Mode and Exit to leave the Menu
- ❖ Save the Changes to return to the Main Display

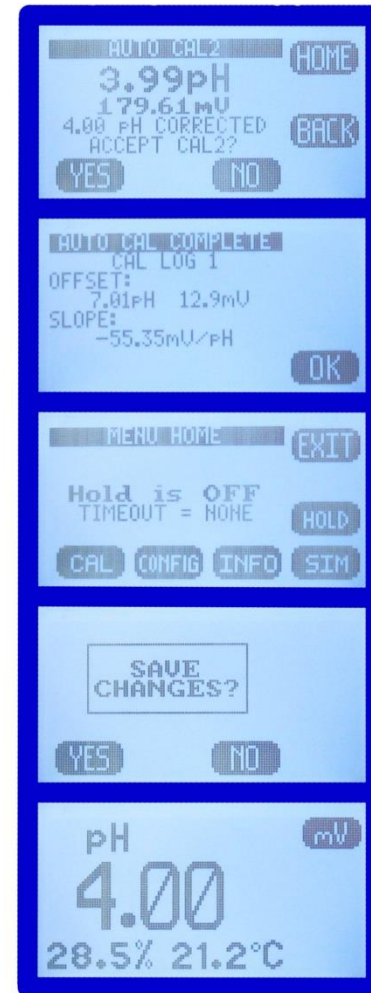

T80 Manual Calibration

- ❖ Manual Calibration allows the Offset and Slope to be entered manually
 - Test an electrode in the shop and install it and enter the Cal Data in the field
- ❖ Enter the PV value, Press mV and enter the associated mV value
- ❖ Accept the entry and enter the slope value
- ❖ Accept the Slope, press OK, Exit and Save the changes

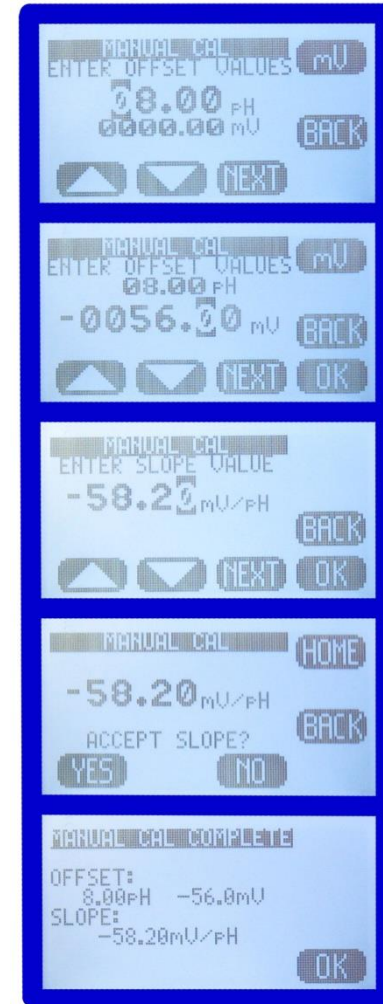




T80 Configure

❖ Configure Transmitter

- LCD – Display
 - Contrast, °C/°F
- OUTPUT
 - 4-20 mA, Relays
- SERIAL
 - MODBUS or HART® addresses
- PASSWORD
 - Set Level and Password

❖ Configure Sensor

- Type of Sensor, pH, ORP...
- Temp Compensation, %/°C
- Isopotential point

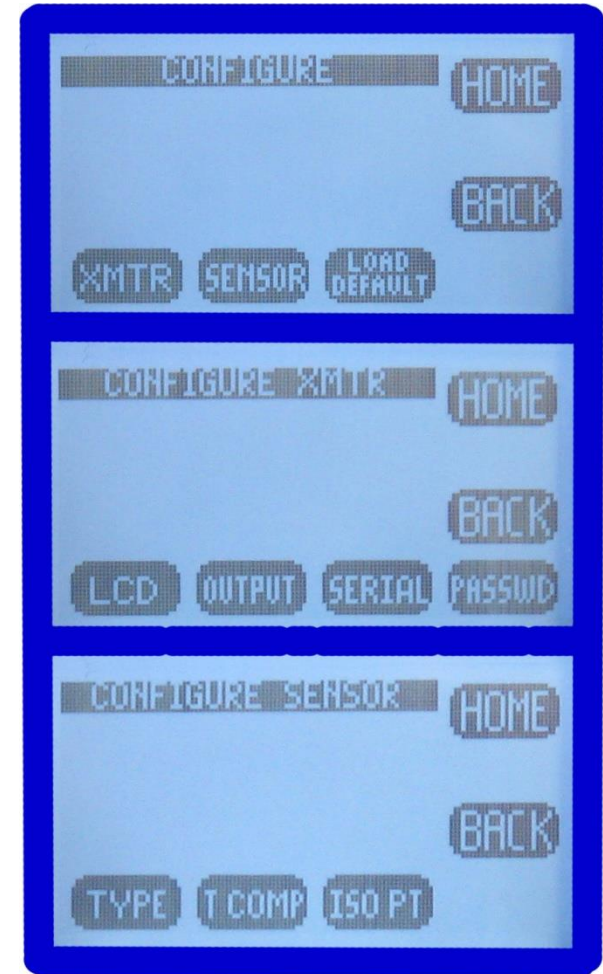


Configure the Display

- ❖ Display Set Up
 - °C or °F
 - Slider for Contrast
 - Time Out for Back Light
- ❖ Soft Keys - Text or Icons
- ❖ Line, Gauge or Bar Graphs
 - Line graph duration
 - 1 minute, 15 minutes, 1 hour, 12 hours, 1 day, 2 days
- ❖ Tag - 52 characters
 - Tag On- Displays Tag in Home screen
 - Pop Up – Turns press twice screen ON/OFF



Configure Outputs - 4-20 mA

- ❖ Set The 4-20 mA RANGE
 - Default setting is the range of the sensor
 - Select 4 mA/20 mA, enter value
 - HOME, EXIT, SAVE
- ❖ Calibrate the Output
 - Transmitter sends out 4 mA signal
 - Enter measured value press OK
 - Transmitter sends out 20 mA signal
 - Enter measured value and press OK
 - Repeat as needed
- ❖ Choose 4-20 mA Fault Condition
 - 3.5 mA
 - 22 mA
 - Disable, none

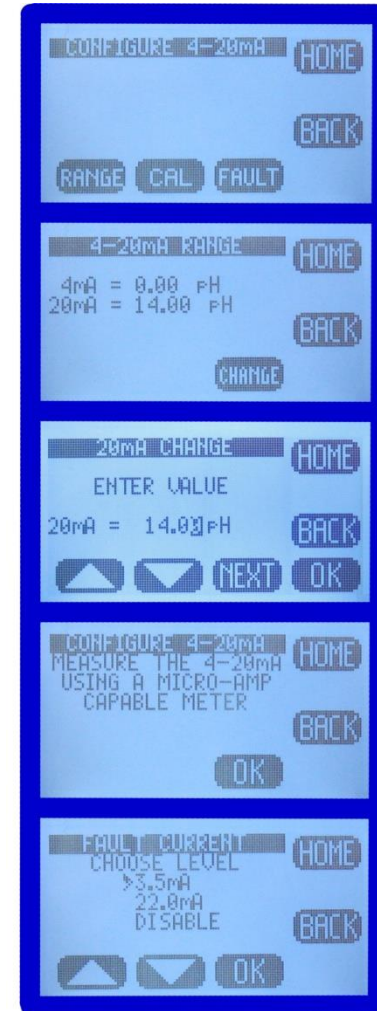

Configure Outputs - Relays


- ❖ 3 Relays
 - SPDT, form 1C, 250 VAC, 5 Amp resistive maximum
- ❖ Choose Relay function
 - Alarm – Set Point
 - Timed – Period & Duration
 - Fault – Failure Alarm
 - Disable – Inactivates relay and removes Icon from Home Display
- ❖ Configure Alarm set point
 - Set Point ON value
 - Expiration, Time the Relay can remain energized
 - Set Point OFF, determines whether Hi/Lo set point
 - Delay Times, Amount of time the PV must stay above or below set point before activation





Hold, Serial, Password

- ❖ Output → Hold
 - Sets the Hold “Time Out” Function
- ❖ Serial Configuration
 - Address (MODBUS + HART®)
 - Baud (MODBUS only)
 - Format (MODBUS only)
- ❖ Password Protection
 - Choose Level
 - Enter 4 character password, case sensitive
 - Master Password in Manual

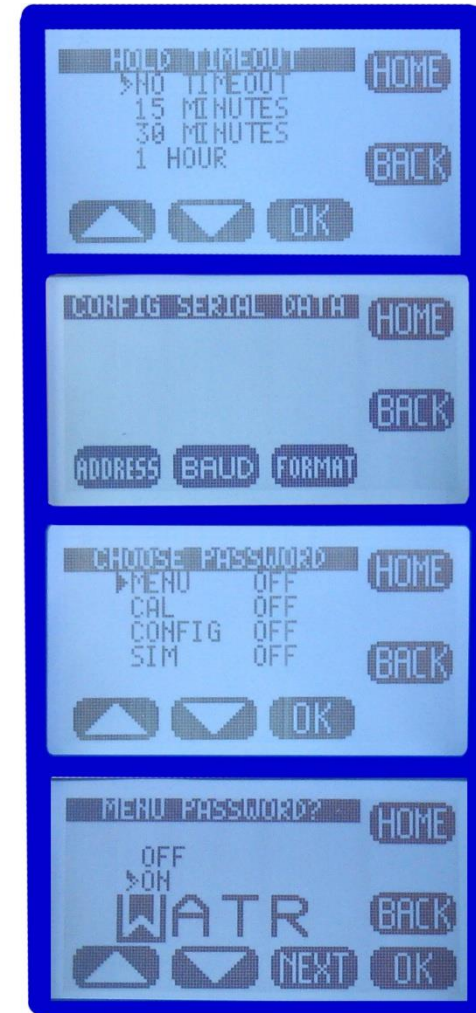

INFO – T80 Transmitter

❖ Transmitter INFO

- Serial #, revision levels, Hardware Software
- T80 Configuration
- Relay configurations 1-3
- 4-20 Configuration





INFO – S80 Sensor

❖ Sensor INFO

- Process Variable, serial #, Firm ware revision
- Sensor's Range
- Calibration Logs
 - Logs 1 – 3
 - Offset & Slope



Simulation - System

❖ System Simulate

- T80 generates a signal equivalent to the PV signal
- Enter Fixed Value
- Ramp (↑ then ↓)
 - Cycles the Range from the low value to the high value and back.
 - Adjustable cycle time
 - Triggers Relays and varies 4-20 mA Out



Simulation – Relays & 4-20 mA

❖ Relay Simulation


- Puts the Relays under manual control
- Choose Relay and turn it ON or OFF

❖ 4-20 mA Simulation

- Enter mA value for T80 to output

❖ That completes the Menus


- CAL
- CONFIG
- INFO
- SIM

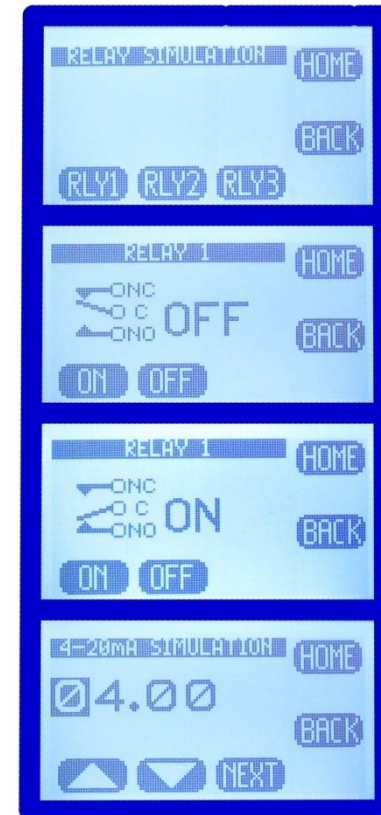

Wiring and Power Board

- ❖ Color Code and Connection type embossed into the protective Circuit Board cover
- ❖ 110/220 VAC Power Board
 - AC In 24 VDC Out
 - Optional preamp for mV+, mV-, TC, TC, SG input





T80 Universal Transmitter

- ❖ One Transmitter for All Measurements
- ❖ Loop Powered, 24 VDC or 110/220 VAC Options
- ❖ HART® 7 or MODBUS RTU
- ❖ With or without 3 Alarm Relays



Model T80 Part Number Guide

Model T80- Transmitter Part Number Guide

Input	10	S80 Sensor, pH, ORP, pION, Conductivity, Resistivity, Turbidity and galvanic Dissolved Oxygen			
	20	Optical DO and Amperometric ppb DO Sensors (Triton® DO8 and DO9 sensors)			
	30	Internal Digital Converter/Preamp			
	Power Supply	-0	Loop Powered Transmitter		
		-1	24 VDC Powered Transmitter		
		-2	110/220 VAC powered Transmitter		
	Alarm Relays	0	No Relays		
			(3) Form 1C, 250 V 5A relays		
		1	Output	0	4-20 mA output and MODBUS RTU
				1	HART®7
				Mounting Hardware	-00 No Mounting Hardware
					-01 Universal Mount
					-02 Panel Mount
					-03 Handrail Mount
					-04 Sunshield Vertical Rail Mount
					-05 Sunshield Horizontal Rail Mount
Model T80-	10	-2	1	1	-01



S80 Intelligent Sensors

- ❖ Noise free digital Communication
- ❖ Calibrated sensors, Plug and Play
- ❖ Easy Maintenance
IP68 Waterproof
Detachable Cable
- ❖ The same Electrode Cartridges, Fittings and Hardware as the S10 and S17 sensors





Electro-Chemical Devices

Thank You,

Go to www.ecdi.com for Data Sheets/ Instruction Manuals/ Presentations/ Press Release Packages

For over 30 years Electro-Chemical Devices (ECD) has been a recognized leader in industrial process instrumentation:

Liquid analytical sensors, controllers, transmitters, analyzers and electrodes.

Electro-Chemical Devices
1500 North Kellogg Dr.
Anaheim, California 92807

Phone: +1-714-695-0051
+1-800-729-1333
Fax: +1-714-695-0057
email: sales@ecdi.com
web: www.ecdi.com

